

(12) INTERNATIONAL APPLICATION PUBLISHED UNDER THE PATENT COOPERATION TREATY (PCT)

(19) World Intellectual Property Organization
International Bureau



(43) International Publication Date
11 December 2003 (11.12.2003)

PCT

(10) International Publication Number
WO 03/102616 A1

(51) International Patent Classification⁷: G01R 33/30,
33/465

(21) International Application Number: PCT/GB03/02372

(22) International Filing Date: 30 May 2003 (30.05.2003)

(25) Filing Language: English

(26) Publication Language: English

(30) Priority Data:
0212581.3 30 May 2002 (30.05.2002) GB

(71) Applicant (for all designated States except US): IM-
PERIAL COLLEGE INNOVATIONS LIMITED
[GB/GB]; Electrical and Electronic Engineering Building,
Imperial College, Exhibition Road, London SW7 2BT
(GB).

(72) Inventors; and

(75) Inventors/Applicants (for US only): KITNEY, Richard,

Ian [GB/GB]; 78 Waldemar Avenue, London SW6 5LU
(GB). GROSS, Patrick [GB/GB]; Imperial College In-
novations Limited, Electrical and Electronic Engineering
Building, Imperial College, Exhibition Road, London SW7
2BT (GB).


(74) Agents: MAGGS, Michael, Norman et al.; Kilburn &
Strode, 20 Red Lion Street, London WC1R 4PJ (GB).

(81) Designated States (national): AE, AG, AL, AM, AT, AU,
AZ, BA, BB, BG, BR, BY, BZ, CA, CH, CN, CO, CR, CU,
CZ, DE, DK, DM, DZ, EC, EE, ES, FI, GB, GD, GE, GH,
GM, HR, HU, ID, IL, IN, IS, JP, KE, KG, KP, KR, KZ, LC,
LK, LR, LS, LT, LU, LV, MA, MD, MG, MK, MN, MW,
MX, MZ, NI, NO, NZ, OM, PH, PL, PT, RO, RU, SC, SD,
SE, SG, SK, SL, TJ, TM, TN, TR, TT, TZ, UA, UG, US,
UZ, VC, VN, YU, ZA, ZM, ZW.

(84) Designated States (regional): ARIPO patent (GH, GM,
KE, LS, MW, MZ, SD, SL, SZ, TZ, UG, ZM, ZW),
Eurasian patent (AM, AZ, BY, KG, KZ, MD, RU, TJ, TM),
European patent (AT, BE, BG, CH, CY, CZ, DE, DK, EE,

[Continued on next page]

(54) Title: DISPOSABLE CONTAINER FOR USE WITH AN OPEN MAGNETIC RESONANCE SCANNER

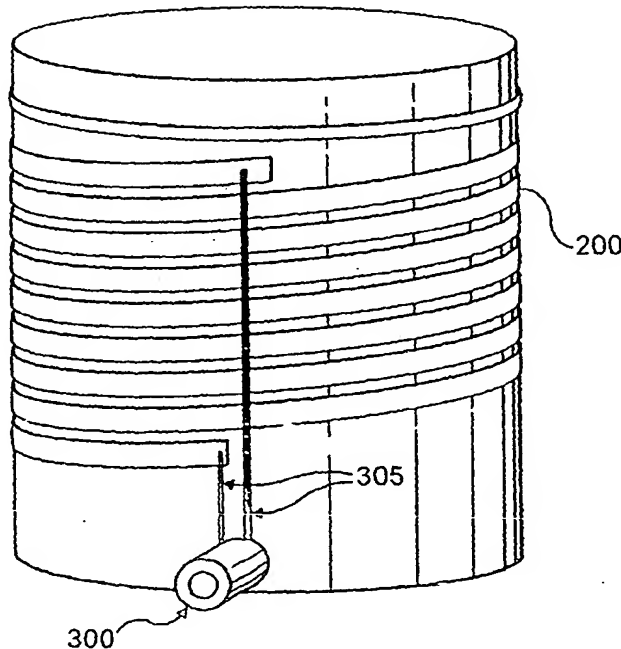

(57) Abstract: A disposable container (100) which can be used to examine excised material during a surgical procedure is adapted for use with an open magnetic resonance scanner. The container (100) has a receive coil (200), provided in or on the body of the container (100), and can be connected (directly or indirectly) to an input of the scanner. During a surgical procedure which is monitored in known manner by magnetic resonance imaging, using the scanner, excised material such as a tumour can be placed in the container and imaged independently to check for example that the tumour and a margin of healthy tissue has been removed. Conveniently, the container can be placed in the field of the open magnetic resonance scanner for imaging, using its receive coil. The container can also be used in magnetic resonance spectroscopy and tumour classification.

WO 03/102616 A1

WO 03/102616 A1



ES, FI, FR, GB, GR, HU, IE, IT, LU, MC, NL, PT, RO,
SE, SI, SK, TR), OAPI patent (BF, BJ, CF, CG, CI, CM,
GA, GN, GQ, GW, ML, MR, NE, SN, TD, TG).

For two-letter codes and other abbreviations, refer to the "Guidance Notes on Codes and Abbreviations" appearing at the beginning of each regular issue of the PCT Gazette.

Published:

— with international search report

DISPOSABLE CONTAINER FOR USE WITH AN OPEN MAGNETIC RESONANCE SCANNER

The present invention relates to a medical analysis device and to methods for fabricating and/or using such a device. It finds particular application in magnetic resonance spectroscopy or imaging, for instance for analysis associated with surgery.

Magnetic resonance imaging ("MRI") for medical diagnosis is well known. Typically, the entire patient or at least that part of the patient to be studied is placed with the main magnetic field of an MRI scanner's magnet. This very strong, homogeneous and static main magnetic field (e.g. 0.5 T) causes the nuclear spins within the patient to align themselves with and against the magnetic field, thereby creating a net magnetic moment in each volume. A transmit coil, typically surrounding the patient, is then used to transmit an excitation pulse which flips the magnetic moment away from its equilibrium position. As the magnetisation decays back to its equilibrium state the spins gyrate around the equilibrium axis and emit signal at the frequency of gyration. This radio frequency signal may be picked up by a receive coil. The frequency of gyration is given by the local magnetic field strength experienced by each spin. This local magnetic field strength is dynamically altered using the scanner's gradients. These superimposed gradients, one in each of the x, y and z directions, typically work at audio frequencies and provide the frequency and phase encoding needed for image reconstruction.

In minimally-invasive MRI, a separate, small, receiving coil or antenna is used to receive the signal, instead of or in addition to the radio-frequency coils of the MRI apparatus itself. Such a coil may be placed either adjacent to the patient's skin or may be inserted by means of a probe into a patient's body cavity, for example into the colon.

MRI is increasingly used during surgical procedures, particularly where tumours or other soft tissue needs to be removed. The area of interest is imaged by the MRI scanner, as surgery proceeds, with both the tumour and the cutting instrument being visible on screen. It is important to remove tumours and their margins without cutting into the affected tissue. Current practice for tumour removal is to mark the tumour boundaries under image guidance (e.g. x-ray, MRI) using markers such as titanium wires, and then to cut around these markers. The result is a lump of tumour, which should have a margin (shell) of healthy tissue surrounding it. It is critical that no off-shoots are missed. Usually this is confirmed by checking that all the markers have been removed and that the tumour is thus completely resected. Furthermore, the operative site is scanned to identify abnormal tissue left and the removed (resected) tissue is placed into a tumour container or resection jar and sent off to a laboratory for further analysis. At the laboratory, x-rays may be taken and frozen sections made.

There are a number of advantages for using MRI for soft tissue imaging. Firstly, the technique does not use ionising radiation. Secondly, no harmful contrast agents are needed. The technique is truly three-dimensional. However, the main advantage is the unrivalled soft-tissue differentiation. MRI may show tumours and tumour margins indistinguishable from healthy tissue in other imaging modality, the naked eye or even to palpation.

In practice, there are a number of problems however. In particular, x-ray analysis of the tumour is not particularly efficient since x-rays do not provide high quality images of soft tissue. Although it would be possible to provide improved images by placing the tumour into another MRI scanner at the laboratory, that would be expensive and would mean either purchasing another

scanner to do the analysis or, alternatively, interrupting the routine of a scanner that would normally be used for scanning patients. Because of the time currently taken to analyse the excised tumour, if any problem is found (for example if only part of the tumour has been excised) the patient typically needs
5 to undergo a further surgical operation. That is clearly undesirable.

In a related use of magnetic resonance, there is also increasing interest in spectroscopy of tumours for tumour classification.

10 According to a first aspect of the present invention, there is provided a container for containing material to be analysed using magnetic resonance, the container including a receive coil for use in analysing material contained in the container.

15 Such a container can be placed within the magnetic field of a magnetic resonance scanner for use during surgery and material which has been removed from a patient can be placed in the container for imaging, during or immediately after a surgical operation, and preferably while it is still available to resume surgery on the patient.

20 Thus, using an embodiment of the present invention, when a tumour is removed it can be placed into the container, within the magnetic field of the MR scanner being used during surgery, allowing the tumour to be imaged there and then, in detail. There are several advantages of such an arrangement.

25 Immediately after the surgical operation has been completed, the surgeon can check whether a tumour has been excised cleanly, with a sufficient margin of healthy material around it. This can be done in the operating theatre, while the patient is still in the scanner and at very little additional cost.

The coil included in the container may also be adapted to act as a transmit coil for use in analysing material contained within the container. In such an arrangement, it may not be necessary that the container be placed in the transmit coil of the MR scanner being used during surgery since the container
5 coil itself, acting in transmit mode might be used to create the necessary excitation pulse. Typically, the container will still be positioned within the main magnetic field and the gradients produced by the MR scanner, since the coil may provide an excitation pulse only without simultaneously being used as a receive coil. However, it would be possible for the coil to be used for both
10 transmit and receive.

Preferably, the container is sealable; it may also have access points (e.g. rubber membranes) for biopsies.

15 Once the surgeon has finished, the container may be sent to a laboratory or other facility for x-rays and/or other analyses to be carried out in the normal way.

Preferably, the container is provided with a connector for connecting the
20 receive coil, directly or indirectly, to an input of a magnetic resonance scanner. In this way, the container can be manufactured as a throw-away item, including just the container with its receive coil and the connector.

In more detail, receive coils for magnetic resonance may in use comprise an
25 inductive part which is connected to circuitry such as matching and decoupling circuits. Preferably, only the inductive part is provided for the container. The more expensive circuitry can be provided as part of the input to a scanner, or as an adaptor for connecting the receive coil to a scanner. The use of an adaptor may be preferred since it supports the use of a single container design with

multiple different scanners and/or field strengths. The adaptor can be scanner-specific while the container is a standard item, without there being any need to manufacture a different container for each model of scanner. Containers may however be manufactured in a variety of shapes and sizes, according to application.

Thus in embodiments of the present invention the design can be flexible. It can use standardised scanner independent parts as throw away items. Expensive and specialised parts can all be multi-use.

10

Preferably, the receive coil is constructed as a volume coil so that material to be imaged can be placed inside the coil. This can provide improved resolution images. Such an arrangement might be particularly suitable for use with an "open" scanner in which patient scans can be carried out during surgical procedures, the surgeon often standing at least partially within the field of the scanner. Open scanners bring huge advantages in guiding the surgeons but current open MRI scanners have low to medium field strengths.

15

The receive coil could be provided in different ways in relation to the container, and could indeed provide at least part of the containment. It could be formed as part of the container body, or it may be added after the container itself has been manufactured. For example, the coil could be created by sputtering techniques, spraying, screen printing, painting etc. To avoid interfering with the scanner's magnetic field, the container, the receive coil and the connector for connecting the receive coil may be made entirely of non-ferromagnetic material.

20

25

According to a second aspect of the present invention, there is provided a scanner for use in analysis by magnetic resonance, the scanner having

detachably connected thereto a container comprising at least in part a receive coil for use in analysing material contained in the container.

5 The scanner may be an open scanner, provided with at least one transmit coil and at least one receive coil which can be arranged for use in imaging the area of a surgical procedure while it is being carried out. The container may be arranged so that it can be disposed in said area to enable analysis of material in the container by use of said at least one transmit coil, together with the receive coil comprised by the container. Alternatively or additionally, the receive coil
10 of the container may also be adapted to function as a transmit coil for use in analysis of material in the container.

An adaptor may be provided between the scanner and the container for adapting the detachable connection to meet requirements of the scanner and of
15 the receive coil of the container in said use in analysing material contained in the container.

According to a third aspect of the present invention, there is provided a method of analysing material by use of magnetic resonance, the method comprising the
20 steps of:

- i) generating a main magnetic field for use in analysing a body of material positioned in the field;
- ii) removing analysed material from said body of material;
- iii) placing the removed material in a container which includes a receive
25 coil, and placing the container in the magnetic field;
- iv) applying an excitation pulse to the removed material; and
- v) using the receive coil of the container in analysing the removed material.

Thus a method of analysis is provided in which some material is analysed twice, using MRI or MRS, once while in a body of material and once again

after being removed therefrom. The second analysis may be carried out next to the body or at some other, second locality remote from a first locality where the body is situated.

- 5 The receive coil of the container might also be adapted to act as a transmit coil, in which case the excitation pulse used for analysis of the material while still in the body of material may be different from the excitation pulse used for analysis of the material after being removed therefrom. However, alternatively, the same excitation pulse could be used for analysis of the
- 10 material while still in the body of material and after being removed therefrom. The main magnetic field is preferably provided by the main magnet of an MRI scanner, with gradients being supplied by the scanner's gradient coils.

According to a fourth aspect of the present invention, there is provided a

15 method of analysing a sample material by use of magnetic resonance, the method comprising the steps of:

- i) placing the sample material in a sample container having a receive coil;
- ii) using a transmit coil external to the container to apply an excitation pulse to the sample material; and
- 20 iii) using the receive coil to analyse the sample material by use of magnetic resonance in response to the excitation pulse.

In this fourth aspect, embodiments of the present invention can provide a method of analysing material by placing the material in a container with a

25 receive coil and putting the container in a magnetic field generated independently and externally (e.g. by a MRI scanner). In such a method, there may be at least two receive coils, a first receive coil for use with the scanner in the normal way, in the absence of the container, and a second receive coil being the receive coil of the container.

In the above, reference is made to "analysis", "analysing" and the like. These are not intended to have any restricted special meaning and should be taken to encompass any operation that might be carried out using magnetic resonance
5 such as imaging, spectroscopy, or characterisation for example, as well as any other suitable form of analysis such as microscopy or biochemical analysis.

Embodiments of the present invention will now be described, by way of example only, with reference to the accompanying drawings in which:
10 Figure 1 shows a resection jar comprising a container according to an embodiment of the present invention;
Figure 2 shows a receive coil for use with the resection jar of Figure 1;
Figure 3 shows a connector for connecting the receive coil of Figure 2 to a scanner input;
15 Figure 4 shows details of an inductively coupled example of the connector of Figure 3;
Figure 5 shows details of a directly coupled example of the connector of Figure 3;
Figure 6 shows a circuit for use with the inductively coupled connector of
20 Figure 4;
Figure 7 shows further coupling circuits; and
Figure 8 shows a cross section of the resection jar of Figure 1 with a sample positioned in the jar for imaging.

25 Referring to Figure 1, the resection jar can be a simple container 100 made of clear material with an o-ring seal 105 and a threaded lid 110. In Figure 1(a), the container 100 is shown open and in cross section, exposing the thread 115 to attach the lid 110 to the body of the container 100. In Figure 1(b), the container 100 is shown closed and in cross section. In Figure 1(c), the

container 100 is shown closed and substantially in side view, in three dimensions.

5 The material of the container 100 is preferably transparent so that the position of a sample in it can be seen. Further, as mentioned above, the container and all its parts should be made entirely of non-ferromagnetic material. For example, the lid and body might be made of perspex or glass. The container may include access points, such as rubber-membrane-covered apertures (not shown) via which biopsies may be taken.

10

Referring to Figure 2, a solenoid coil 200 is wound onto the outside of the container 100 using for example adhesive copper tape. Solenoid coils are simple and give a good homogeneous magnetic field. The coil 200 could be used as a receive-only antenna, or as a transmit/receive antenna. As the scanner's main magnetic field needs to be perpendicular to the solenoid coil's axis, the configuration is well suited for scanners with horizontal magnetic fields and this includes most scanners. For scanners with vertical fields, the container 100 could either be turned onto its side, or a different configuration could be used.

20

Referring to Figure 3, it is necessary to connect the ends of the coil 200 to a connector 300 for connecting the container to a scanner for use. This can be done using enamelled copper wire 305 which is stripped at the contact points and soldered to the ends of the coil 200. It is then attached to the connector 300.

25

Referring to Figure 4, depending on the material of the container, the connector 300 could be glued to or screwed into the container 100. Figure 4 shows a version in which a screw 400 is used. It might be necessary to use several

screws. The ruggedness of the mounting would need to be adapted to suit the proposed use of the container. At the end of assembly, the entire container 100 is coated with an epoxy resin or other insulating, sealing and hardening varnish.

5 Referring to Figures 4 and 5, at least two different options exist for the design of the connector 300. The first option is to use inductive coupling, as shown in Figure 4. The second option is to use a direct connection, as shown in Figure 5. A third option would be to connect the coil to the scanner by means of a wireless connection using a transmitter and receiver, ensuring that the transmitted signal does not interfere with the operation of the scanner, and vice versa. An example of such a wireless link is a connection by means of an infrared optical signal.

15 Taking the first option, the connector 300 shown in Figure 4(a) provides the socket of a plug and socket arrangement. The plug component 405 is shown in Figure 4(b) and the two parts are shown coupled together and held by an O-ring 420 in Figure 4(c). The socket 300 and the plug component 405 each contain a coaxial solenoid 410, 415 and their mutual inductance is used to transfer energy from the solenoid coil 200 towards the scanner. To put it another way, the solenoid 410 adds to or forms part of the coil inductance.

25 Taking the second option, as shown in Figure 5(a), the connector 300 again provides the socket of a plug and socket arrangement but this time it is equipped with two pairs of resilient conductive blades 500. A plug component 405 for this form of the connector 300 is shown in Figure 5(b) and this is equipped with two conductive prongs 505 which can be pushed between the conductive blades 500 to complete the coupling, as shown in Figure 5(c). Each conductive prong 505 couples to a wire 305 such as is shown in Figure 3.

Both types of coupling are known per se, inductive and direct. Figures 6 and 7 show the circuitry suggested by each respectively. Such circuitry might be provided at an input to a scanner, or (preferably) as part of an adaptor for connecting the container 100 to a scanner. The adaptor will typically be proximal to the container.

The circuits of Figures 6 and 7 are disclosed in "An inductively coupled, series-tuned NMR probe", *M. Decords, P. Blondet, H. Reutenauer, J.P. Albrand Journal of Magnetic Resonance 65, 100-109 (1985).*

Referring to Figure 6, for the inductively coupled circuit the container 100 will have to have a mounted capacitor C_s . Ideally it should be chosen to match a given field strength. However, it is also possible to use the same container for a range of field strengths, making more extensive provisions on the socket side. Figures 6(a) and 6(b) show equivalent circuits. At the socket side, we have control over L_p , r_p , C_m and M . Typically, r_p should be roughly zero, and M should be high. M , L_p and C_m may be adjusted to achieve matching.

Referring to Figure 7a, from the circuit point of view, the direct contact arrangement shown in Figure 5 is simpler. The container 100 need not have any components mounted other than the coil 200 and it may be used for all field strengths.

A decoupling scheme may need to be added if the coil 200 on the container 100 is to be used as receive only. This may be achieved using a DC bias on the coaxial cable to switch a diode at the input terminals of the matching section, as is shown in Figures 7(b) and 7(c).

Referring to Figure 8, material 800, 805 such as foam, preferably non-water-absorbing, may be inserted in the container 100 to ensure correct positioning of the sample 810 in the container 100. Once the sample 810 is positioned inside the container, the container can be sealed and/or labelled inside the operating theatre, facilitating transport of the sample to a second site, such as a laboratory, for storage or further analysis. This is particularly relevant in case that the second site is located in a different part of the hospital where the operating theatre is located, or in an entirely different building.

Various design features may be preferred for use of the container 100. For instance, it may be preferred that the base of the container is made anti-slip and a label area might be provided on the outside. The entire container is preferably disposable and intended for single-use only. Alternatively, the container may be made of suitable materials to allow sterilisation and re-use.

In the above, attention is given to imaging of material, particularly to support surgical procedures. However, there may be other applications to which embodiments of the invention would be relevant. An example of one of these is magnetic resonance spectroscopy of tumours for tumour classification.

CLAIMS:

1. A container for containing material to be analysed using magnetic resonance, the container including a receive coil for use in analysing material
5 contained in the container and a connector for detachably connecting the receive coil, directly or via an adaptor, to an input of a magnetic resonance scanner.
2. A container according to Claim 1, wherein the connector provides an
10 inductive coupling to the receive coil.
3. A container according to Claim 1, wherein the connector provides a direct electrical contact to the receive coil.
- 15 4. A container according to Claim 1, wherein the connector includes a transmitter for establishing a wireless link between the receive coil and the input of the magnetic resonance scanner.
- 20 5. A container according to any one of claims 1 to 3 wherein the receive coil is also adapted for use as a transmit coil for use in analysing material contained in the container.
6. A container according to any one of the preceding claims wherein the
25 container is sealable.
7. A container according to any one of the preceding claims wherein the receive coil is constructed as a volume coil such that material to be analysed can be placed inside the coil.

8. A container according to any one of the preceding claims wherein the container is made of non-ferromagnetic material such that material contained in the container can be analysed by use of an excitation pulse generated by use of at least one transmit coil external to the container.

5

9. A scanner for use in analysis by magnetic resonance, the scanner having detachably connected thereto a container including a receive coil for use in analysing material contained in the container.

10

10. A scanner according to Claim 9, said scanner being an open scanner, provided with at least one transmit coil and at least one receive coil arranged for use in imaging a three-dimensional space in which a surgical procedure can be at least partially carried out.

15

11. A scanner according to Claim 10 wherein the container is disposed in said space to enable analysis of material contained in the container by use of said at least one transmit coil, together with the receive coil of the container.

20

12. A scanner according to any one of Claims 9, 10 or 11 wherein the receive coil of the container is adapted to function additionally as a transmit coil for use in analysis of material contained in the container.

25

13. A scanner according to any one of Claims 9 to 12, the scanner being provided with an adaptor between the scanner and the container, for adapting the detachable connection to meet requirements of the scanner and of the receive coil of the container in said use in analysing material contained in the container.

14. A method of analysing material by use of magnetic resonance, the method comprising :

- i) generating a main magnetic field for use in analysing a body of material positioned in the field;
- 5 ii) removing analysed material from said body of material;
- iii) placing the removed material in a container which includes a receive coil; and
- iv) placing the container in the magnetic field;
- v) applying an excitation pulse to the removed material; and
- 10 vi) using the receive coil of the container in analysing the removed material.

15. A method according to Claim 14 wherein the body is at least initially situated in a first locality; the method further comprising

- vii) sealing the container at the first locality.

15

16. A method according to Claim 14 wherein the body is at least initially situated in a first locality; the method further comprising

- viii) labelling the container at the first locality.

20 17. A method according to Claim 14 wherein the body is at least initially situated in a first locality; the method further comprising

- ix) transporting the container to a second locality.

25 18. A method according to Claim 14 wherein the body is at least initially situated in a first locality; the method further comprising

- x) further analysing the removed material at a second locality.

19. A method according to Claim 14 wherein the receive coil of the container is adapted also to act as a transmit coil, for generating the excitation pulse.

5 20. A method according to claim 14 wherein the excitation pulse is generated by a transmit coil external to the container.

21. A method according to claim 14 wherein the body is a patient and the first locality is an operating theatre.

10

22. A method of analysing body tissue by use of magnetic resonance, the method comprising :

- i) generating a main magnetic field for use in analysing a body tissue of a patient positioned in the field;
- 15 ii) resecting the analysed body tissue from said patient;
- iii) placing the resected body tissue in a container which includes a receive coil; and
- iv) placing the container in the magnetic field;
- v) applying an excitation pulse to the resected body tissue; and
- 20 vi) using the receive coil of the container in analysing the resected body tissue.




23. A method according to Claim 22, wherein the patient is situated in an operating theatre.

25

24. A method according to Claim 23 further comprising
vii) sealing the container inside the operating theatre.

25. A method according to Claim 23 further comprising
viii) labelling the container inside the operating thratre.
26. A method according to Claim 23 further comprising
5 ix) further analysing the resected body tissue outside the operating thratre.
27. A method according to Claim 22 wherein the receive coil of the
container is adapted also to act as a transmit coil, for generating the excitation
pulse.
10
28. A method according to claim 22 wherein the excitation pulse is
generated by a transmit coil external to the container.
29. A method according to claim 22, wherein the body tissue comprises
15 tumour tissue
30. A method of analysing a sample material at a first locality by use of
magnetic resonance, the method comprising the steps of:
i) placing the sample material in a sample container having a receive coil;
20 ii) using a transmit coil external to the container to apply an excitation
pulse to the sample material; and
iii) using the receive coil to analyse the sample material by use of magnetic
resonance in response to the excitation pulse.
- 25 31. A method as claimed in claim 30 further comprising
iv) sealing the container at the first locality.
32. A method as claimed in any of claims 30 to 31 further comprising
v) labelling the container at the first locality.

33. A method as claimed in any of claims 30 to 32 further comprising
vi) transporting the container to a second locality.
34. A method as claimed in any of claims 30 to 32 further comprising
5 vii) further analysing the sample material at a second locality.
35. A method as claimed in any of claims 30 to 34 including using
apparatus external to the container to provide a main magnetic field within
which the sample container is positioned during analysis.
10
36. A method as claimed in any of claims 30 to 35 including using
apparatus external to the container to provide magnetic gradients within which
the sample container is positioned during analysis.
- 15 37. A method as claimed in any of claims 30 to 36, wherein the sample
material comprises body tissue.
38. A method as claimed in any of claims 30 to 37, wherein the sample
material comprises tumour tissue.
20
39. A method as claimed in any of claims 30 to 38, wherein the first locality is
an operating theatre.
40. A method as claimed in claims 33 or 34, wherein the second locality is a
25 laboratory.

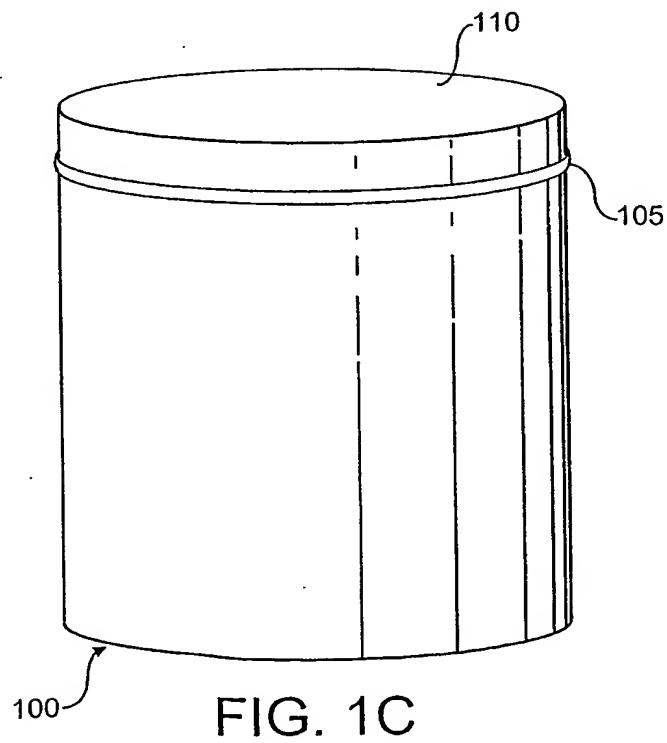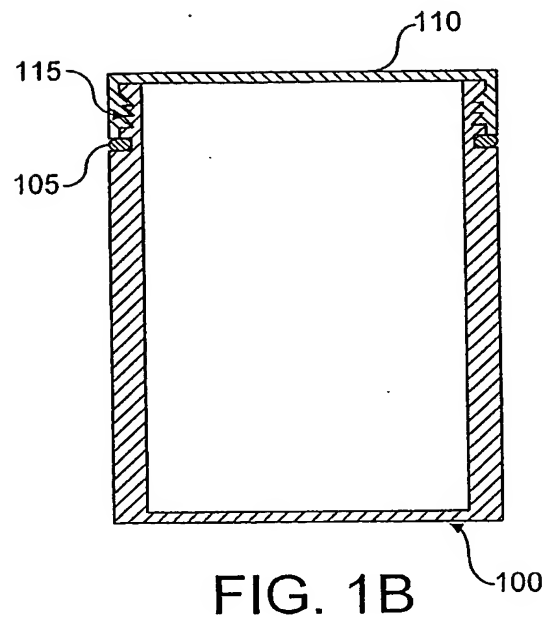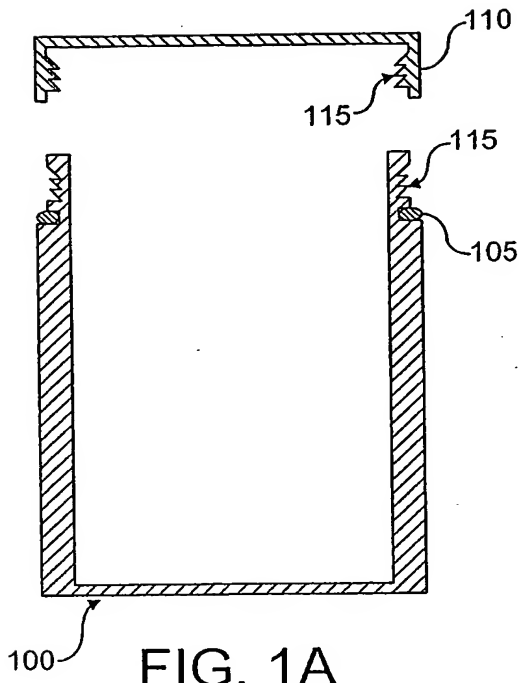

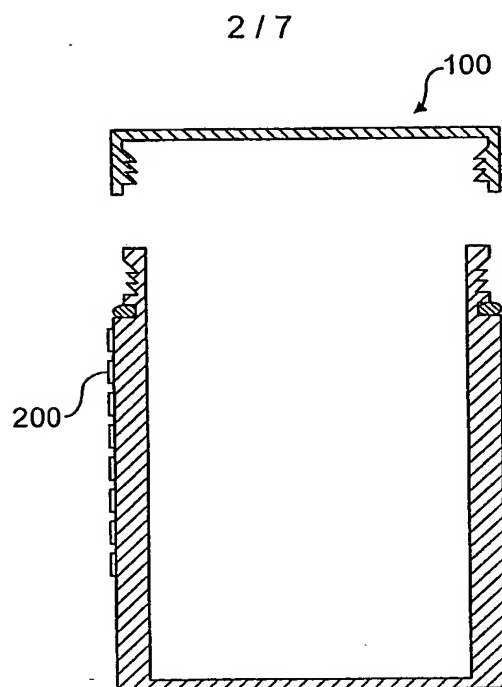


FIG. 2A

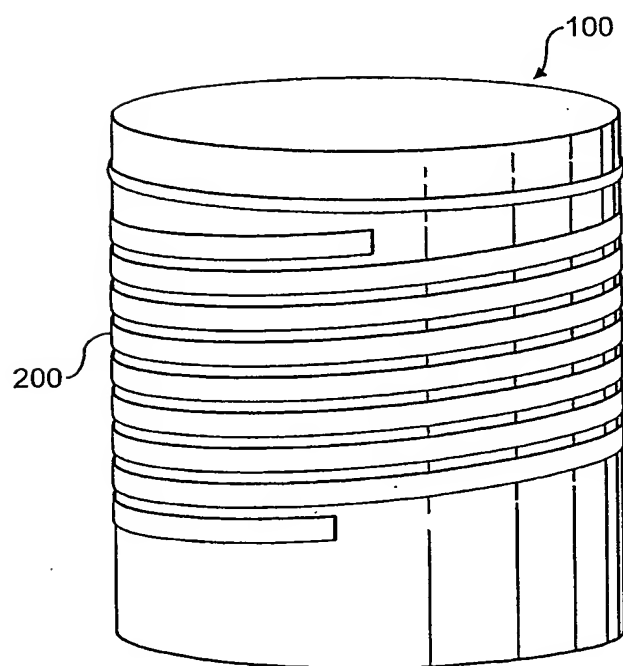


FIG. 2B

3 / 7

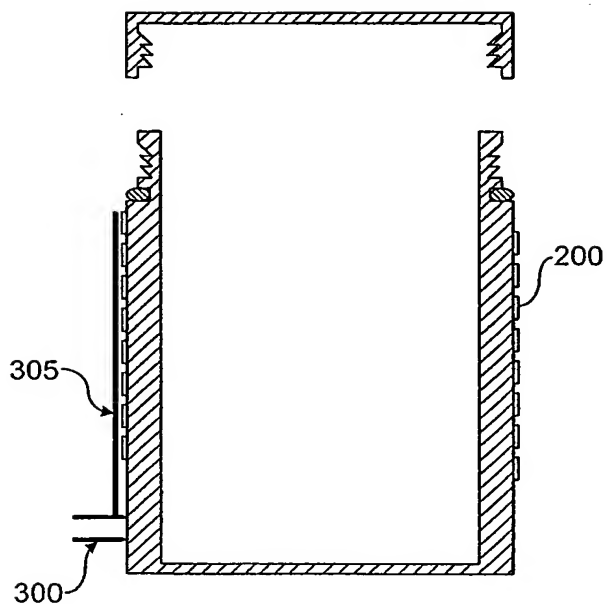


FIG. 3A

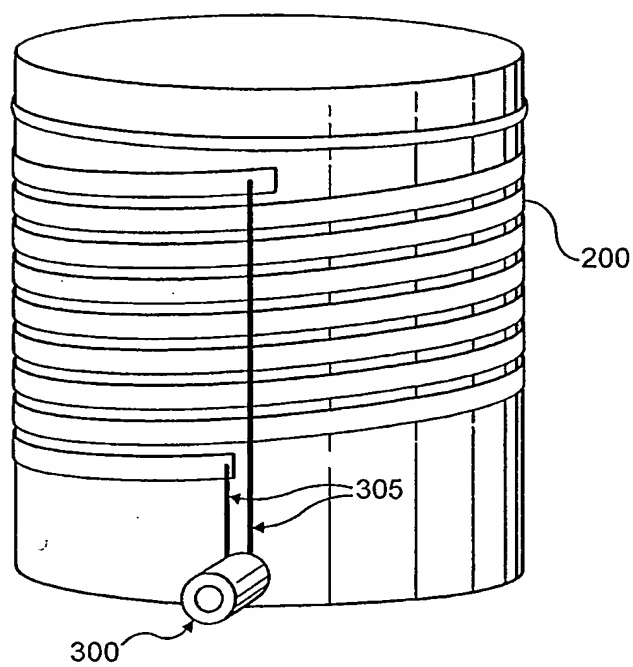


FIG. 3B

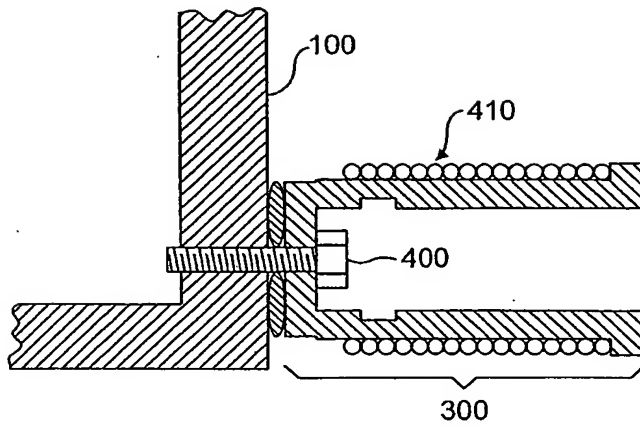


FIG. 4A

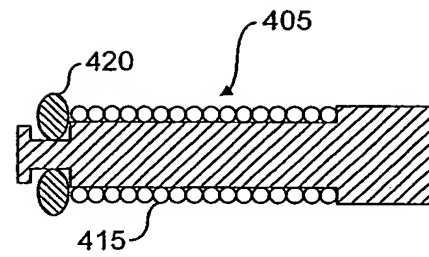


FIG. 4B

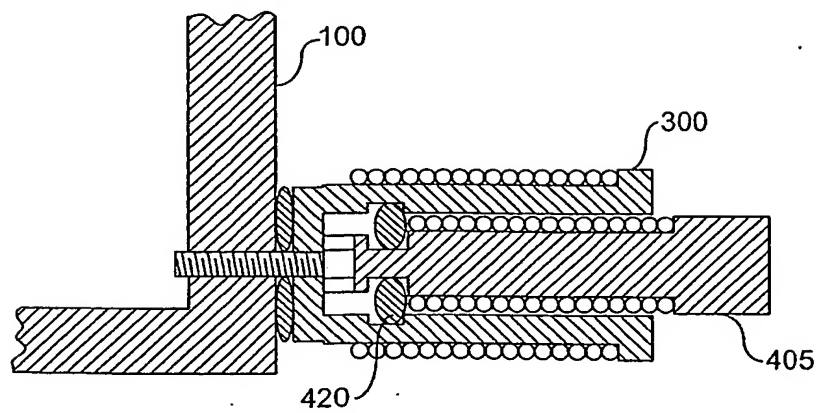
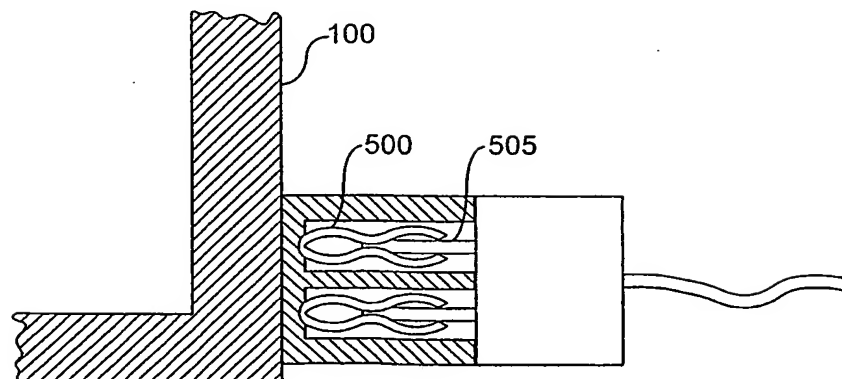
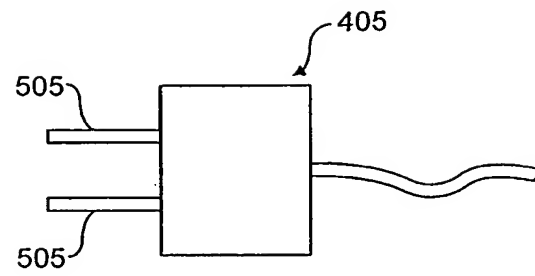
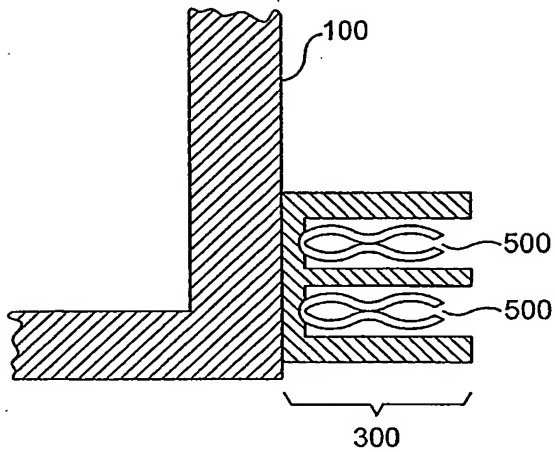


FIG. 4C



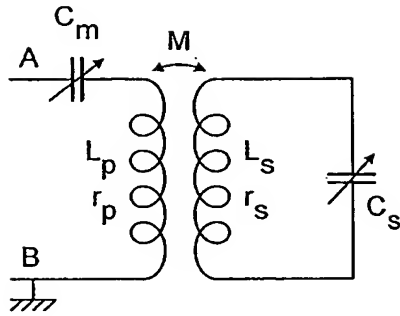


FIG. 6A

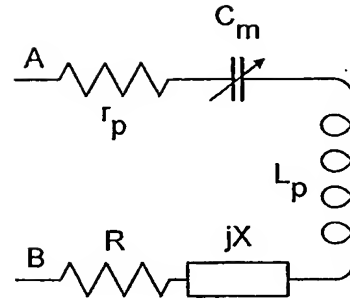


FIG. 6B

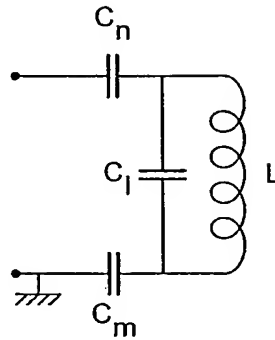


FIG. 7A

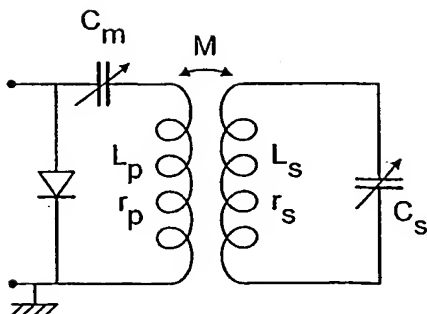


FIG. 7B

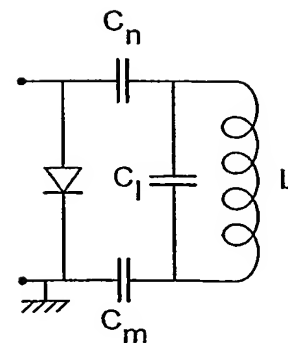


FIG. 7C

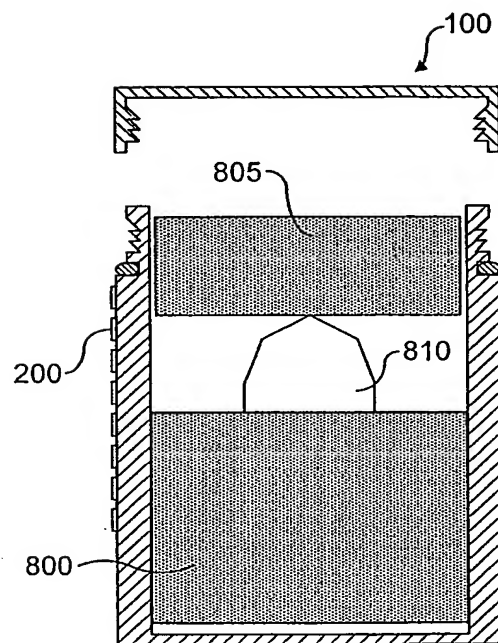


FIG. 8

INTERNATIONAL SEARCH REPORT

International Application No
PCT/GB 03/02372A. CLASSIFICATION OF SUBJECT MATTER
IPC 7 G01R33/30 G01R33/465

According to International Patent Classification (IPC) or to both national classification and IPC

B. FIELDS SEARCHED

Minimum documentation searched (classification system followed by classification symbols)
IPC 7 G01R G01N

Documentation searched other than minimum documentation to the extent that such documents are included in the fields searched

Electronic data base consulted during the international search (name of data base and, where practical, search terms used)

EPO-Internal, PAJ, WPI Data, INSPEC, BIOSIS, EMBASE, MEDLINE

C. DOCUMENTS CONSIDERED TO BE RELEVANT

Category *	Citation of document, with indication, where appropriate, of the relevant passages	Relevant to claim No.
X	EP 0 346 049 A (GEN ELECTRIC) 13 December 1989 (1989-12-13) column 7, line 6 - line 11; claims 1,2; figure 4	1,3,5, 7-9,12 2,4
Y	---	
Y	EP 0 468 857 A (MAGNETECH S A) 29 January 1992 (1992-01-29) column 8, line 53 -column 9, line 25	2
Y	---	
Y	US 5 245 288 A (LEUSSLER CHRISTOPH G) 14 September 1993 (1993-09-14) column 1, line 26 - line 54	4
X	---	
X	US 4 184 110 A (HINSHAW WALDO S) 15 January 1980 (1980-01-15) column 5, line 2 - line 25; figure 2	1,5,7-12

	-/--	

☒ Further documents are listed in the continuation of box C.☒ Patent family members are listed in annex

* Special categories of cited documents:

- *A* document defining the general state of the art which is not considered to be of particular relevance
- *E* earlier document but published on or after the international filing date
- *L* document which may throw doubts on priority claim(s) or which is cited to establish the publication date of another citation or other special reason (as specified)
- *O* document referring to an oral disclosure, use, exhibition or other means
- *P* document published prior to the international filing date but later than the priority date claimed

- *T* later document published after the international filing date or priority date and not in conflict with the application but cited to understand the principle or theory underlying the invention
- *X* document of particular relevance; the claimed invention cannot be considered novel or cannot be considered to involve an inventive step when the document is taken alone
- *Y* document of particular relevance; the claimed invention cannot be considered to involve an inventive step when the document is combined with one or more other such documents, such combination being obvious to a person skilled in the art.
- *A* document member of the same patent family

Date of the actual completion of the international search

14 August 2003

Date of mailing of the international search report

02/09/2003

Name and mailing address of the ISA

European Patent Office, P.B. 5818 Patentlaan 2
NL - 2260 HV Rijswijk
Tel (+31-70) 340-2040, Tx. 31 651 epo nl,
Fax (+31-70) 340-3016

Authorized officer

Skalla, J

INTERNATIONAL SEARCH REPORT

Internat~~l~~ Application No
PCT/GB 03/02372

C.(Continuation) DOCUMENTS CONSIDERED TO BE RELEVANT		
Category *	Citation of document, with indication, where appropriate, of the relevant passages	Relevant to claim No.
X	US 4 875 485 A (MATSUTANI KINYA) 24 October 1989 (1989-10-24) column 5, line 27 - line 43 -----	1,3,5, 7-12
X	EP 0 750 188 A (DIRECTOR GENERAL OF NATIONAL A) 27 December 1996 (1996-12-27) column 3, line 27 - line 43 column 5, line 41 - line 55 column 8, line 4 - line 17 -----	1,3,5, 7-9,12
X	BALLON D ET AL: "RESOLUTION ENHANCED NMR SPECTROSCOPY IN BIOLOGICAL SYSTEMS VIA MAGNETIC SUSCEPTIBILITY MATCHED SAMPLE IMMERSION CHAMBERS" MAGNETIC RESONANCE IN MEDICINE, ACADEMIC PRESS, DULUTH, MN, US, vol. 30, no. 6, 1 December 1993 (1993-12-01), pages 754-758, XP000416462 ISSN: 0740-3194 page 755, left-hand column, last paragraph -right-hand column, paragraph 2; figure 2A -----	1,6
X	PATENT ABSTRACTS OF JAPAN vol. 011, no. 022 (P-538), 21 January 1987 (1987-01-21) & JP 61 196145 A (TOSHIBA CORP), 30 August 1986 (1986-08-30) abstract -----	1
X	GRANT D.M., HARRIS R.K. : "Encyclopedia of Nuclear Magnetic Resonance" 1996, JOHN WILEY & SONS, CHICHESTER XP002251232 * Cozzone P.J. et al, "Tissue & Cell Extracts MRS", p. 4771-4775* -----	14-35, 37-40
A	US 5 550 471 A (FELD PETER) 27 August 1996 (1996-08-27) column 1, line 19 -column 2, line 6 -----	1,3

INTERNATIONAL SEARCH REPORT

Information on patent family members

International Application No

PCT/GB 03/02372

Patent document cited in search report		Publication date	Patent family member(s)	Publication date
EP 0346049	A	13-12-1989	US 4885539 A	05-12-1989
			EP 0346049 A2	13-12-1989
			IL 90127 A	01-12-1992
			JP 2043706 A	14-02-1990
			JP 2058773 C	10-06-1996
			JP 5061761 B	07-09-1993
EP 0468857	A	29-01-1992	FR 2665265 A1	31-01-1992
			EP 0468857 A1	29-01-1992
			JP 6054824 A	01-03-1994
US 5245288	A	14-09-1993	DE 4126537 A1	11-02-1993
			DE 59207884 D1	27-02-1997
			EP 0527530 A1	17-02-1993
			JP 3187152 B2	11-07-2001
			JP 5261085 A	12-10-1993
US 4184110	A	15-01-1980	GB 1601816 A	04-11-1981
			DE 2822953 A1	30-11-1978
			JP 1425448 C	15-02-1988
			JP 54001686 A	08-01-1979
			JP 62031295 B	07-07-1987
			NL 7805815 A	29-11-1978
US 4875485	A	24-10-1989	JP 1626776 C	28-11-1991
			JP 2052498 B	13-11-1990
			JP 62117541 A	29-05-1987
			DE 3639140 A1	21-05-1987
EP 0750188	A	27-12-1996	JP 9005317 A	10-01-1997
			EP 0750188 A1	27-12-1996
			US 5759797 A	02-06-1998
JP 61196145	A	30-08-1986	NONE	
US 5550471	A	27-08-1996	DE 4337908 A1	11-05-1995
			JP 7184880 A	25-07-1995